



Disclaimer: unless otherwise agreed by the Council of UPOV, only documents that have been adopted by the Council of UPOV and that have not been superseded can represent UPOV policies or guidance.

This document has been scanned from a paper copy and may have some discrepancies from the original document.

---

Avertissement: sauf si le Conseil de l'UPOV en décide autrement, seuls les documents adoptés par le Conseil de l'UPOV n'ayant pas été remplacés peuvent représenter les principes ou les orientations de l'UPOV.

Ce document a été numérisé à partir d'une copie papier et peut contenir des différences avec le document original.

---

Allgemeiner Haftungsausschluß: Sofern nicht anders vom Rat der UPOV vereinbart, geben nur Dokumente, die vom Rat der UPOV angenommen und nicht ersetzt wurden, Grundsätze oder eine Anleitung der UPOV wieder.

Dieses Dokument wurde von einer Papierkopie gescannt und könnte Abweichungen vom Originaldokument aufweisen.

---

Descargo de responsabilidad: salvo que el Consejo de la UPOV decida de otro modo, solo se considerarán documentos de políticas u orientaciones de la UPOV los que hayan sido aprobados por el Consejo de la UPOV y no hayan sido reemplazados.

Este documento ha sido escaneado a partir de una copia en papel y puede que existan divergencias en relación con el documento original.

UPOV

TC/XVIII/11

ORIGINAL: English

DATE: November 3, 1982

## INTERNATIONAL UNION FOR THE PROTECTION OF NEW VARIETIES OF PLANTS

GENEVA

## TECHNICAL COMMITTEE

Eighteenth Session  
Geneva, November 18 and 19, 1982

COLOR MEASUREMENTS

document prepared by the Office of the Union

The Annex to this document, reproducing a letter from Mr. Espenhain (Denmark) dated October 26, 1982, and addressed to the Office of UPOV, contains the information on the colorimeter VIPDENS 501. This information may be of value for the discussions under item 4 of the draft Agenda of the eighteenth session of the Technical Committee (document TC/XVIII/1), of the proposals for establishing a UPOV Color Chart.

[Annex follows]

PLANTENYHEDSNÆVNET

Teglværksvej 10 - Tystofte 0346

DK-4200 Skælskør

Telefon (03) 596141

TC/XVIII/11

ANNEX

26. October 1982

PN/82 - 447

UPOV

34, chemin des Colombettes

1211 Genève 20

Att: Senior Counsellor M.-H. Thiele-Wittig

Dear Mr. Thiele-Wittig,

Re: The session in Technical Committee next month  
- Color Measurement.

With reference to the observations concerning various Color Measurements given during the Council session this month I forward you as agreed more information on the colorimeter VIPDENS 501.

As I informed you, one of our institutes (The Research Laboratory for the Fruit- and Vegetable Industry) is testing the said colorimeter at the moment and makes comparison studies between the VIPDENS and the previously used colorimeter, Hunterlab.

As it can be read in the 'User Manual' enclosed, the colorimeter is of pocket size and the reading aperture is 3 mm compared with the Hunterlab.'s 2-4 cm. The price is approx. 1,550 Sch.fr. compared with the price of the Hunterlab. at approx. 48,000 Sch.fr.

The said laboratory has agreed that Plantenyhedsnævnet as formerly may also use the new colorimeter and we plan to do this in the examination of *Euphorbia pulcherrima* Willd. ex Klotzsch. The experience gained will be made available to The Technical Working Party for Ornamentals next year.

In a workshop within the EEC Agrofood Programme concerning quality in apples, which took place in Milan 6.-9. July this year, the participating experts decided to recommend to their respective authorities the purchase of the VIPDENS colorimeter, if possible. I include this information as it might be possible that experiences gained in other countries could be made available as well.

Furthermore I can inform you that the laboratory in question is working on a mathematical conversion formula which will make it possible to compare the results from the VIPDENS and Hunterlab. colorimeters and therefore also the RHS color chart.

To the extent you wish you may copy the 'User Manual' for inclusion in the document you are preparing for the Technical Committee.

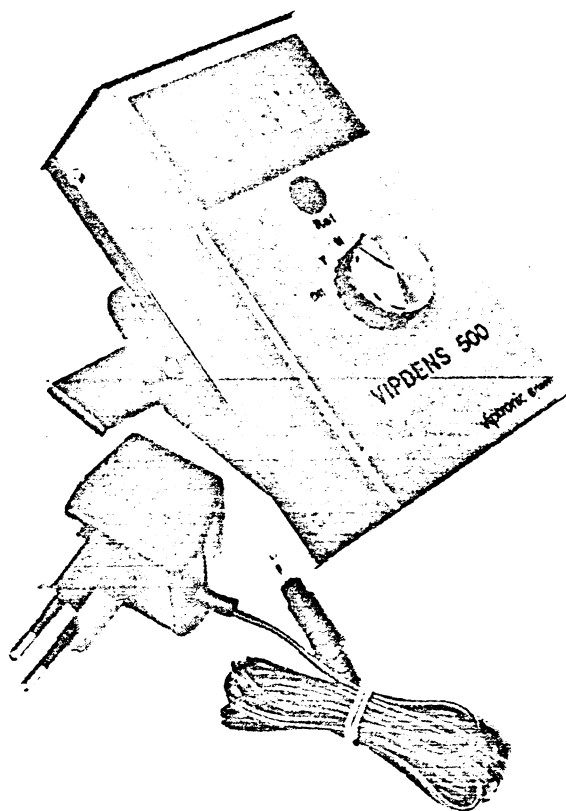
Yours sincerely,

P. n. v.

  
Flemming Espenhain

**USER MANUAL  
BEDIENUNGSANLEITUNG****VIPDENS 500**

**VIPTRONIC GmbH  
BRIXEN - ITALY  
I-39042 Brixen  
Fischzuchtweg 2  
Tel. (0472) 24122**

**SPECIFICATIONS:**

Range:	D 0,00 - D 2,50
Linearity:	$\pm$ D 0,01
Repeatability:	$\pm$ D 0,01
Accuracy:	$\pm$ D 0,01
Digital display (height):	13 mm
Reading aperture:..	3 mm $\varnothing$
Battery (rechargeable):	9 V
Dimensions:	135 x 78 x 40 mm

NOTE: B/W-version available!

## INTRODUCTION

The VIPDENS 500 colour reflection densitometer is a instrument of very advanced design. Use of the most modern electronic developments has provided the VIPDENS 500 with exceptionally high linearity and stability as well as extraordinary reliability and compactness. Cordless operation, by use of a rechargeable battery, and a large liquid crystal digital display open new fields of application wherever colour reflection densitometry is required. The colour measurement filters conform to the DIN 16536 standard «colour density measurements on prints». For the yellow channel a special glass interference filter is employed which increases the range for the yellow readings to more nearly match those of the other colours. By comparison, densitometers employing the commonly used blue filter (Wratten no. 47 or equivalent) typically produce density readings up to 0.38 lower in the yellow channel than the VIPDENS 500.

## CALIBRATION

The VIPDENS 500 is very strictly calibrated logarithmically in manufacture and conforms to the internationally used 10-step «quantalog check plaque». Because of the extreme stability of the VIPDENS 500 no further calibration is necessary.

Whilst not recommended, it is possible to co-ordinate the readings of the VIPDENS 500 with another densitometer having a non standard slope; if required this procedure is obtainable from your next authorized VIPTRONIC agent.

## ZEROING

The VIPDENS 500 has a push-button zero function which will store the exact values for the particular «paper white» in use. These values remain stored in the instrument's memory, even when it is switched off, until replaced with new values by repeating the zeroing procedure.

## ZEROING PROCEDURE

1. Switch instrument on by turning rotary switch to «Y» (yellow). Check that red indicator on left of digital display does not light indicating low battery charge - see sect. «BATTERY».
2. Release base plate lock (left-hand side of unit) by pulling outwards and raise reading head.
3. Locate area representative of «paper white» and place reading aperture over it. Steady the instrument by holding the extended base plate locking lever with left hand.
4. Press button «Ref.» and while keeping it pressed lower the densitometer head to the reading position. **Important:** The head should be held down in the reading position with the «Ref.» button pressed until the yellow indicator light goes out. This takes about 1.3 seconds and ensures that the reading has entered the instrument's memory (RAM).
5. Raise the reading head. The «Y» (yellow) channel is now zeroed.

The «M» (magenta) channel is zeroed in the same way by turning the rotary switch to «M» and repeating steps 2 to 5. Also the «C» (cyan) and «B» (black) channels.

Remember that these values will remain stored in the instrument's memory when switched off, even for long periods, until replaced by new values from another zeroing procedure.

The VIPDENS 500 will zero automatically, as above, on paper stocks with densities up to 0.7 from «standard white».

Readings of 9.99, 9.98 etc. indicate densities of .01 and .02 respectively whiter than the sample used to zero the instrument.

**COLOUR DENSITY READINGS**

After the VIPDENS 500 has been zeroed in all channels on the paper stock in use, colour density readings are made as follows:

1. Release base plate lock.
2. Turn rotary switch to ink colour to be read (Y = yellow, M = magenta, C = cyan, B = black).
3. Place reading aperture over sample, making sure that entire area of the 3.5 mm  $\phi$  aperture is filled. Hold instrument firmly in position with left hand on extended locking plate lever.
4. Lower reading head to reading position and hold it there until yellow lamp (LED) extinguishes (about 1.3 secs.) indicating that the reading is complete. Raise the reading head.
5. The density of the sample will be shown on the liquid crystal display, and remains until another channel is selected and a reading made, or the instrument is switched off.
6. Readings of the other colours are made by selecting the appropriate channel and repeating steps 3 to 5.

**BATTERY**

The VIPDENS 500 densitometer is powered by a rechargeable nickel-cadmium battery of 110 mA/h capacity, delivering 9 Volts d.c. Depending on the reading technique, up to 5000 readings can be made from a fully charged battery. A major contribution to extended battery life is made by the instrument's design which automatically switches the sample illumination lamp off after each reading (when the yellow LED goes out).

In the upper part of the window to the left of the LCD display is a red indicator lamp which illuminates to warn of low battery charge. If this lamp lights continuously the instrument should be recharged before use, otherwise spurious readings may result.

To recharge the VIPDENS 500 the battery charger (supplied) is plugged into the socket marked «Battery» on the lower side of the instrument and the charger plugged into a 240 V a.c. power socket; the recharging time for a completely exhausted battery is c. 14 hours. Longer times will not harm the battery but care must be taken to ensure that the recharging time does not exceed 30 hours.

If the red indicator lamp lights only during a reading, work with the instrument may continue with the charger connected as above. If a great many readings are to be made daily from a fixed location, the VIPDENS 500 may be operated with the charger connected continuously.

It is important to remember that once the red indicator lights continuously the instrument cannot produce accurate readings whether the charger is connected or not.

The battery's efficiency can be impaired by accidental over charging or by leaving it in a discharged state for long periods. A symptom of deteriorating battery efficiency is frequent need of recharging, or in extreme cases the red indicator light remaining on after recharging. In this case the battery should be replaced by removing the two screws securing the lower end plate («Battery») of the instrument and unplugging the battery. It should be replaced with a nickel-cadmium accumulator conforming to IEC 6F22; suitable types are available from numerous manufacturers including Varta (T7/8), ITT (T9) and General Electric.

**Important:** Never short circuit an accumulator, puncture the casing or dispose of in a fire!

**SOME TIPS ON GETTING THE BEST FROM YOUR VIPDENS 500**

1. Always keep the battery adequately charged.
2. Do not release densitometer head from reading position until reading is complete as indicated by yellow lamp.
3. Allow at least one second interval between readings.
4. Use only the recharging unit supplied with the VIPDENS 500.
5. Clean the measuring aperture and optic system when necessary with a cotton tipped stick slightly moistened with water. Do not use any other cleaning materials.
6. Do not press down hard on densitometer when making readings.